
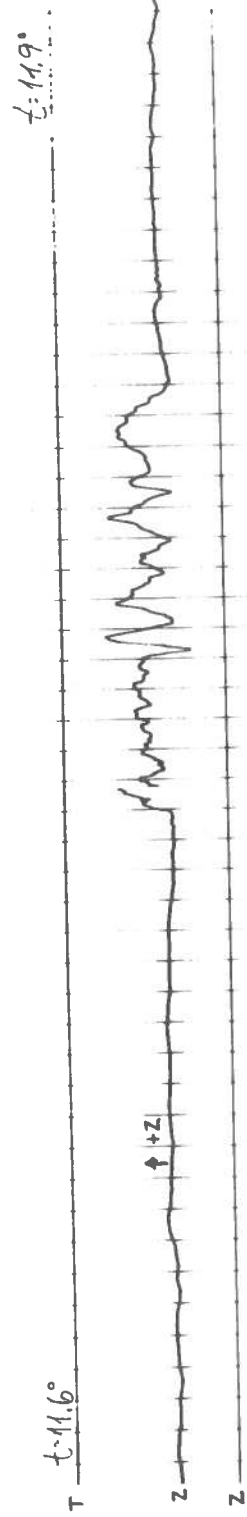
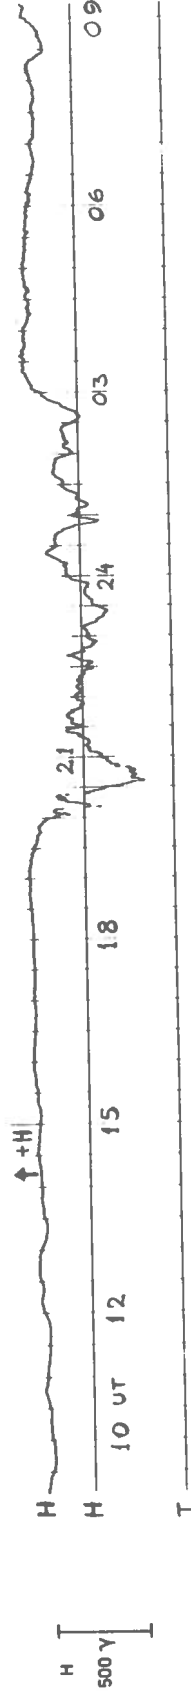


FORMAT FOR STORM MAGNETOGRAMS
(SAMPLE ONLY)

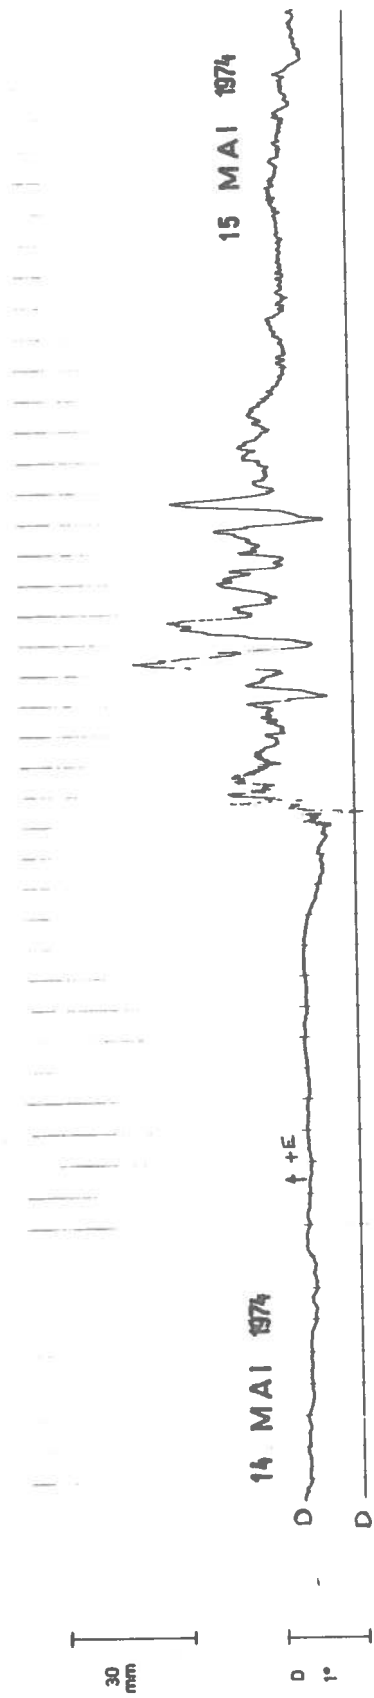

SEE CALIBRATION DATA FOR SCALE VALUES AND BASELINE VALUES

NORMAL MAGNETOGRAPH					
COMPONENT	PERIOD		CALIBRATION		
	FROM	TO	SCALE VALUE	BASELINE	TEMP. COEFF.
D	1. Feb.	28. Feb.	1.45' /mm	1.0' E	
H	1. Feb.	28. Feb.	5.28 nT/mm	11203 nT	+8.5 nT/C ^o
Z	1. Feb.	6. Feb.	6.50 nT/mm	51515 nT	-2.8 nT/C ^o
	7. Feb.	8. Feb.	"	51503 nT	"
	9. Feb.	28. Feb.	"	51485 nT	"

STORM MAGNETOGRAPH					
COMPONENT	PERIOD		CALIBRATION		
	FROM	TO	SCALE VALUE	BASELINE	TEMP. COEFF.
D	1. Feb.	28. Feb.	3.0' /mm	52.0' W	
H	1. Feb.	28. Feb.	22.2 nT/mm	11140 nT	-0.8 nT/C ^o
Z	1. Feb.	28. Feb.	24.0 nT/mm	51188 nT	-3.7 nT/C ^o

PRELIMINARY QUIET MEAN ABSOLUTE VALUES		
D	H	Z
35.5' E	11370 nT	51570 nT
Computed from following days: 10. 14. 18. 19. 21.		